



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷ : G01N 33/543, 27/00	A1	(11) International Publication Number: WO 00/14539 (43) International Publication Date: 16 March 2000 (16.03.00)
(21) International Application Number: PCT/GB99/02952 (22) International Filing Date: 6 September 1999 (06.09.99) (30) Priority Data: 9819319.6 5 September 1998 (05.09.98) GB (71) Applicant (for all designated States except US): AEA TECHNOLOGY PLC [GB/GB]; 329 Harwell, Didcot, Oxfordshire OX11 0RA (GB). (72) Inventors; and (75) Inventors/Applicants (for US only): SOFIELD, Carl, John [GB/GB]; Gage Cottage, Rowstock, Didcot, Oxfordshire OX11 0JS (GB). MORGAN, George, Richard [GB/GB]; 10 Broadway close, Harwell, Didcot, Oxfordshire OX11 0LB (GB). HARPER, Ruth, Elizabeth [GB/GB]; Gage Cottage, Rowstock, Didcot, Oxfordshire OX11 0JS (GB). STOCKFORD, Gavin, John [GB/GB]; 10 Hampden Road, Cowley, Oxford, Oxfordshire OX4 3LW (GB). (74) Agents: MANSFIELD, Peter, Turquand et al.; AEA Technology plc, Patents Dept., 329 Harwell, Didcot, Oxfordshire OX11 0RA (GB).		(81) Designated States: AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, US, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG). Published <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i>
(54) Title: ASSAY OF CHEMICAL BINDING USING MICRO-CANTILEVERS		
(57) Abstract <p>A method of comparing the binding strengths of a plurality of different ligands to a receptor, in which several micro-cantilever structures (10) are coated with the receptor on at least a part of a surface (13) of each micro-cantilever structure (10). Each micro-cantilever structure (10) is then contacted with a different ligand solution, and the amounts by which the micro-cantilever structures deflect are compared. The deflection may be detected by an optical lever (16, 18; 28). The micro-cantilever structures (10) may be in the form of an array, each structure (10) being in a respective well (24), to which ligand solutions are added.</p>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav	TM	Turkmenistan
BF	Burkina Faso	GR	Greece		Republic of Macedonia	TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's	NZ	New Zealand		
CM	Cameroon		Republic of Korea	PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

ASSAY OF CHEMICAL BINDING USING MICRO-CANTILEVERS

This invention relates to a method and an apparatus for assaying chemical binding, that is to say reversible reactions between a receptor and a ligand.

Micro-cantilevers such as those used in atomic force microscopy have recently been suggested for use in other applications, for example being sensitive to temperature. It has been suggested that measurements may be based on either the frequency of vibration, or the bending of the micro-cantilever. For example the force of adhesion between the tip of a micro-cantilever derivatized with avidin, and agarose beads functionalized with biotin, has been measured by Florin et al. (Science, April 1994, 264 p. 415). The use of a micro-cantilever to observe changes in surface stress has been described by H. J. Butt (Journal of Colloid and Interface Science 180 (1996) pp. 251-260). A micro-cantilever will bend if the surface stress on one face changes, and this change might for example be caused by a change of pH or of salt concentration if one face of the micro-cantilever is coated with a different material to the opposite face. Butt suggests that such a micro-cantilever may be used to monitor concentrations of substances in the medium around the cantilever, or to measure the specific binding of ligands to cantilevers which are coated on one side with a receptor. However he advises that any such measurements should be performed in a flow-through manner, and his measurements (for example with changing pH) indicate that there is a delay of some minutes before the micro-cantilever responds, so such a process would require significant quantities of reagents; furthermore the relationship with concentration is not clear, as the

bending was observed to depend linearly on salt concentration, but also to vary approximately linearly with pH - which is a logarithmic function of concentration.

5

According to the present invention there is provided a method of comparing the binding strengths of a plurality of different ligands to a receptor, the method comprising coating a plurality of micro-cantilever structures with the receptor, the coating being applied to at least a part of a surface of each micro-cantilever structure, contacting each micro-cantilever structure with a different ligand solution, and comparing the amounts by which the micro-cantilever structures deflect when contacted with the respective ligand solutions.

This method enables you to determine which of the ligands binds most strongly to the given receptor, and so to assay the different ligands in relation to that receptor. Hence the method enables specific binding with any one of the ligands, if it occurs, to be detected, so enabling that ligand to be identified. Equally it enables the binding of the different ligands to the receptor to be ranked in order of strength. Measurements of deflection with different concentrations of the same ligand may also enable the equilibrium constant, K , for the binding reaction to be determined.

The invention also provides an apparatus for performing this method, the apparatus incorporating an array of such micro-cantilever structures, and means to measure how much the structures deflect. Deflection of the structures may be detected optically, for example by reflecting light from a reflective portion of the micro-

cantilever structure onto a position-sensitive photodiode.

The micro-cantilever structures are desirably all of the same size. Each may be in the form of a rectangular strip of length less than 0.5 mm, and typically of length between 0.1 and 0.4 mm, fixed at one end, and of thickness typically less than 0.001 mm, for example 0.6 microns. They may be of V shape, and the width of each arm (or of the cantilever) is typically less than a fifth of its length. They may be made of materials such as silicon nitride, silicon, or polymers. Because of their small size their natural frequency of vibration can exceed 10 kHz, so they respond rapidly and are not much affected by noise (which tends to be of lower frequencies). The coating of such micro-cantilevers with a chromium layer followed by a gold layer is known, this improving the optical reflectivity of the coated surface so that deflection or bending of the micro-cantilever can be detected optically, for example with an optical lever. The gold layer can be further coated with organic chemicals, for example with long-chain alkanethiols (e.g. octadecanethiol), as such thiols form self-assembled, highly ordered, stable monolayers on gold.

A potential problem with such micro-cantilevers is that temperature changes can also cause bending. This may be prevented by ensuring the temperature does not change significantly during measurements. Preferably each micro-cantilever structure incorporates means to enable deflections due to ligand-receptor binding to be distinguished from those due to other causes of bending (such as vibration, or temperature). Such common mode noise rejection may be achieved using a V shape micro-

cantilever coated with the organic receptor material on just one arm, so that ligand-receptor binding causes twisting of the micro-cantilever rather than bending (and temperature changes cause bending rather than twisting).
5 Such twisting has a higher resonant frequency than bending, which further suppresses the effect of noise. Twisting may be detected more easily by providing a cross piece integral with the V shaped micro-cantilever. An alternative embodiment uses two adjacent rectangular
10 micro-cantilevers whose free ends are linked by a torsion bar. - Another alternative uses two adjacent micro-cantilevers just one of which is coated with the organic receptor material, and the difference in the bending of the two micro-cantilevers is determined.

15 The micro-cantilevers might be coated with organic receptor molecules using the thiol approach described previously, or by means of an interposed bonding layer as described in GB 2 225 963 B. The bonding layer may
20 comprise a silylating reagent, such as $R_3Si(CH_2)_nNH_2$, which can be connected to a protein by bonding the amino group ($-NH_2$) to a carboxylic acid group; as in that patent, R can be O-alkyl, O-aryl, O-heterocyclic, alkyl, aryl, or heterocyclic, and n may be zero or any integer.
25 The receptor molecules may then be treated with an initial ligand of moderate binding strength, such that only those ligands under test which bind more strongly (and therefore displace the initial ligand) cause deflection of the micro-cantilever structure.

30

Different coating processes may be suitable for applying other receptor molecules. For example the

coating may be deposited by Langmuir-Blodgett film transfer, which forms a monomolecular layer.

The method may comprise arranging an array of micro-
5 cantilever structures so that each micro-cantilever structure is immersed in a respective vessel of water, and then adding solutions of the ligands to each of the vessels and observing the effect on each of the micro-cantilever structures. The addition may cause vibration
10 of the micro-cantilever, but this is only transient. Thus by using an array of for example 200 micro-cantilever structures and 200 corresponding vessels, the strength of bonding of 200 different potential ligands to a given receptor can be compared simultaneously. Each vessel
15 must be large enough to accommodate a micro-cantilever structure, but can therefore be as small as a 1 mm cube, or even smaller. In an alternative method each micro-cantilever structure is in a respective flow channel, through which different solutions are caused to flow.
20

The deflection of each micro-cantilever structure can be related to the equilibrium constant K for the ligand-receptor binding reaction, and hence to the change of free energy for that reaction. The rate constant for
25 adsorption cannot usually be measured, because the rate of change of deflection of the micro-cantilever structure is usually limited by the diffusion of ligand through the water rather than by the rate of adsorption; however if the concentration is sufficiently high and the size of
30 the vessel is sufficiently small then the rate of adsorption can also be determined. The rate constant for desorption may be measured using the flow channel method, initially contacting a micro-cantilever with a ligand solution so that binding occurs, and then contacting it

with pure water so that desorption can occur (the water flushing away any desorbed ligand molecules).

The invention will now be further and more particularly described, by way of example only, and with reference to the accompanying drawings, in which:

Figure 1 shows a plan view of a micro-cantilever;

10 Figure 2 shows a view in the direction of arrow 2 of figure 1;

Figure 3 shows a sectional view of apparatus incorporating an array of micro-cantilevers;

15

Figure 4 shows graphically the variation of deflection with time of a micro-cantilever as a result of a ligand-receptor binding reaction;

20 Figure 5 shows graphically the variation of deflection with time where two different ligands bind successively to a receptor; and

Figure 6 shows graphically the variation of
25 deflection with time where a micro-cantilever is exposed to different concentrations of a ligand.

Referring to Figure 1, a micro-cantilever 10 is fixed at one end to a block 12. The micro-cantilever 10
30 is generally V-shaped in plan, comprising two converging strips 13,14, which are integral with a transverse cross strip 15. It projects 0.2 mm from the block 12, the strips 13 and 14 each being 24 microns wide and the entire micro-cantilever 10 is of silicon nitride of

thickness 0.6 microns. The top surface of the micro-cantilever 10 is coated with a 5 nm layer of chromium followed by a 13 nm layer of gold, to improve its optical reflectivity. The gold on one strip 13 is then coated
5 with octadecanethiol, which forms a self-assembled, highly ordered monolayer on gold, and biotin is then bonded to this monolayer. Biotin acts as a selective receptor for avidin.

10 Application of a coating of receptor molecules on just one strip 13 may be achieved by coating just that strip with gold (by masking the other strip 14); or by coating both strips 13 and 14 with gold and with receptor molecules, and then removing the receptor molecules from
15 one strip 14 for example by ozone and ultraviolet irradiation, or by using a laser (with masking of the other strip 13).

Referring now to Figure 2, any deflection or
20 twisting of the micro-cantilever 10 is detected optically, by focusing a light beam from a laser diode 16 onto the cross strip 15, and detecting the reflection with a quadrant photodiode 18. The light intensities detected by the four segments of the photodiode 18 may be
25 used to determine the deflection of the cross strip 15. If the micro-cantilever 10 is exposed to a solution of avidin, which binds to the biotin, this changes the surface stress of the strip 13, causing the micro-cantilever 10 to twist, so changing the inclination of
30 the cross strip 15.

Referring now to Figure 3, test equipment 20 comprises a silicon wafer 22 defining an array of through holes 24 each of diameter 0.7 mm. Within each hole 24 is

a micro-cantilever 10 with gold on its lower surface. A thin glass plate 26 is bonded to the lower surface of the wafer 22, so that an array of liquid vessels are defined by the holes 24 and the plate 26. Deflection of the
5 micro-cantilevers 10 is detected by shining a beam of light onto the lower surface of the glass plate 26, and detecting the movement of the reflected spots of light. In use of the equipment 20, the gold surface of each micro-cantilever 10 is coated with the same receptor
10 (e.g. biotin), and water is placed in each vessel 24. Solutions of different ligands are then injected into each vessel, a different ligand into each vessel, so that the degree to which each ligand bonds to that receptor can be ranked.

15

Referring now to Figure 4, this shows graphically the variation with time of the deflection (in arbitrary units) of the micro-cantilever 10 when immersed in water in a small vessel of volume 0.4 ml, before and after
20 injecting avidin into the water. After injection, the concentration of avidin is 0.08 μM . The time at which the avidin is injected is indicated by the arrow A. Before this time the deflection is substantially constant. The injection causes a transient oscillation followed by a
25 gradual change in deflection over a period of about five minutes, the deflection then reaching a new, steady value differing by h from its initial value. The bending is caused by the surface stress change resulting from the reaction; the change in surface stress is, at least
30 approximately, equal to the change of surface energy, which can be related to the concentration c of the ligand and the equilibrium constant K of the binding reaction onto the surface (i.e. k_a/k_d , where k_a is the adsorption

coefficient and k_d is the desorption coefficient).
Consequently the deflection h is given by:

$$h = C \ln(1 + cK)$$

5

where C is a constant.

Referring now to Figure 5, this shows graphically the variation with time of the deflection (in arbitrary units) of the micro-cantilever 10 when immersed in water in the small vessel. At the time indicated by the arrow P immunoglobulin G (IgG) was injected, and at the time indicated by the arrow Q avidin was injected. As with the results shown in Figure 4, after each injection the deflection gradually changes over a period of several minutes before reaching a new steady value. In this case the deflection resulting from the immunoglobulin was about 200 units, and addition of avidin - which binds to biotin more strongly - led to a further deflection of about 200 units. The avidin displaces the immunoglobulin G which has bound to the biotin, because it binds more strongly.

Referring now to Figure 6, this shows graphically the variation with time of the deflection (in arbitrary units) of the micro-cantilever 10 when immersed in water in the small vessel. At the time indicated by the arrow R immunoglobulin G (IgG) was injected so the concentration in the vessel was $0.047 \mu\text{M}$, and at the time indicated by the arrow S additional immunoglobulin G (IgG) was injected to raise the concentration to $0.088 \mu\text{M}$. The deflection resulting from the initial injection (after about 10 minutes) was about 235 units, whereas the deflection resulting from the second injection was about

- 10 -

290 units (after a further 10 minutes). As expected from the equation for h given above, in a case such as this where the equilibrium constant is large (say 10^9 l/mole), the deflection does not increase linearly with
5 concentration.

It will be appreciated that the process might be modified in various ways while remaining within the scope of the invention. A variety of different ways of bonding
10 the receptor to the micro-cantilever structure may be used instead of the long chain alkane thiol approach described previously. An alternative bonding molecule would comprise a long chain alkane having a thiol group near one end and a carboxylic acid group near the other
15 end, i.e. COOH-R-SH , where the thiol group would be bonded to the gold layer; the carboxylic acid group might then be bonded to a protein. An alternative bonding layer is a silylating reagent as described in GB 2 225 963 B. The micro-cantilever structures might be of a different
20 shape to that described above, for example comprising two adjacent rectangular micro-cantilevers whose free ends are linked by a torsion bar; movement of the torsion bar might be detected optically or capacitively.

25 It is desirable to coat the surface of the micro-cantilever 10 opposite that on which is the coating of receptor molecules, to suppress any potential biochemical interactions at that surface. Diamond-like carbon is a suitable coating for this purpose. This can for example
30 be deposited, in a vacuum chamber, by exposing those surfaces to a vapour of a hydrogenated carbonaceous material (such as polyphenyl ether) while subjecting the

surfaces to bombardment by ions of say oxygen or nitrogen of energy in the range 40 - 80 keV.

Claims

1. A method of comparing the binding strengths of a plurality of different ligands to a receptor, the method
5 comprising coating a plurality of micro-cantilever structures with the receptor, the coating being applied to at least a part of a surface of each micro-cantilever structure, contacting each micro-cantilever structure with a different ligand solution, and comparing the
10 amounts by which the micro-cantilever structures deflect when contacted with the respective ligand solutions.
2. A method as claimed in claim 1 wherein each micro-cantilever structure is of length less than 0.5 mm, of
15 thickness less than 0.001 mm, and is fixed at one end.
3. A method as claimed in claim 1 or claim 2 wherein each micro-cantilever structure is of V shape, and the width of each arm is less than a fifth of its length.
20
4. A method as claimed in claim 3 wherein the organic receptor is coated on just one arm of each micro-cantilever structure, so that ligand-receptor binding causes twisting of the micro-cantilever structure.
25
5. A method as claimed in claim 1 or claim 2 wherein each micro-cantilever structure comprises two adjacent rectangular micro-cantilevers whose free ends are linked by a torsion bar.
30
6. A method as claimed in any one of the preceding claims wherein each micro-cantilever structure is coated with the receptor by means of an interposed bonding layer.

7. A method as claimed in claim 6 wherein the bonding layer comprises $R_3Si(CH_2)_nNH_2$, wherein R is O-alkyl, O-aryl, O-heterocyclic, alkyl, aryl, or heterocyclic, and n
5 is zero or any integer.

8. A method as claimed in any one of the preceding claims wherein the receptor is treated with an initial ligand of moderate binding strength, such that only those
10 ligands under test which bind more strongly cause deflection of the micro-cantilever structure.

9. A method as claimed in any one of the preceding claims comprising arranging an array of micro-cantilever
15 structures so that each micro-cantilever structure is immersed in a respective vessel of water, and then adding solutions of the ligands to each of the vessels and observing the effect on each of the micro-cantilever structures.

20

10. An apparatus for performing a method as claimed in any one of the preceding claims, the apparatus including an array of micro-cantilever structures, and means to measure deflection of those structures.

Fig. 1.

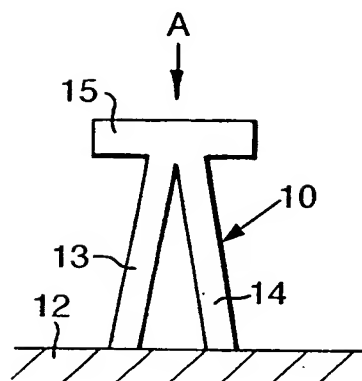


Fig. 2.

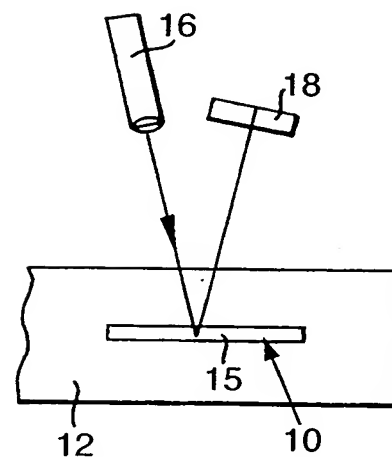


Fig. 3.


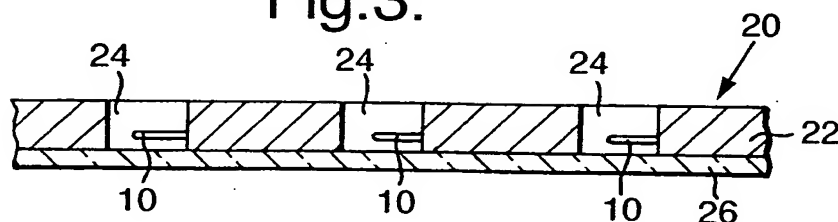


Fig. 4.

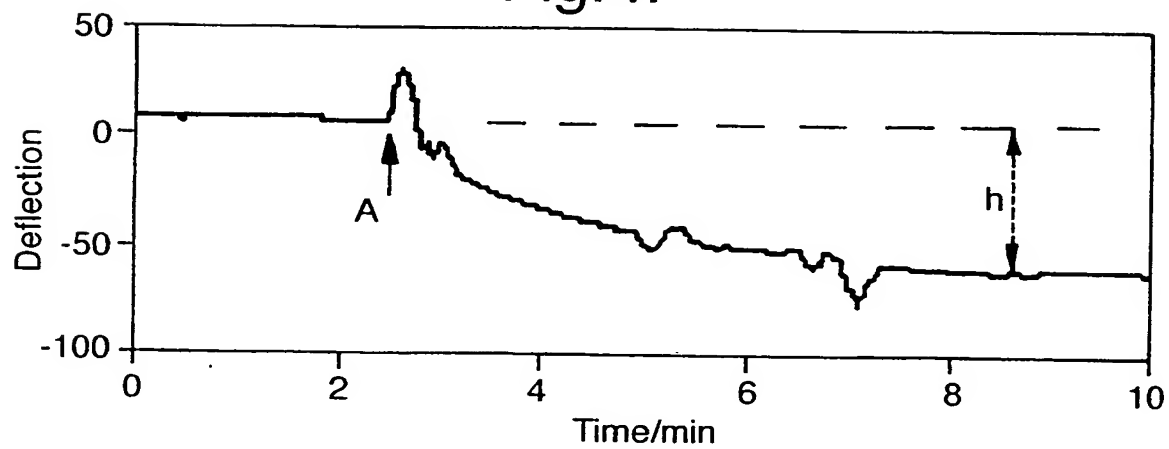


Fig.5.


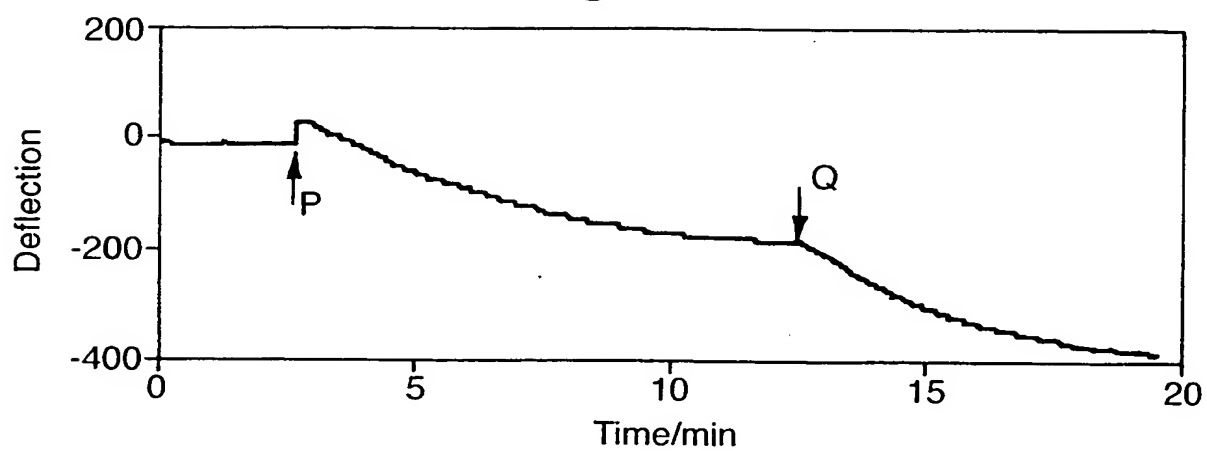


Fig.6.

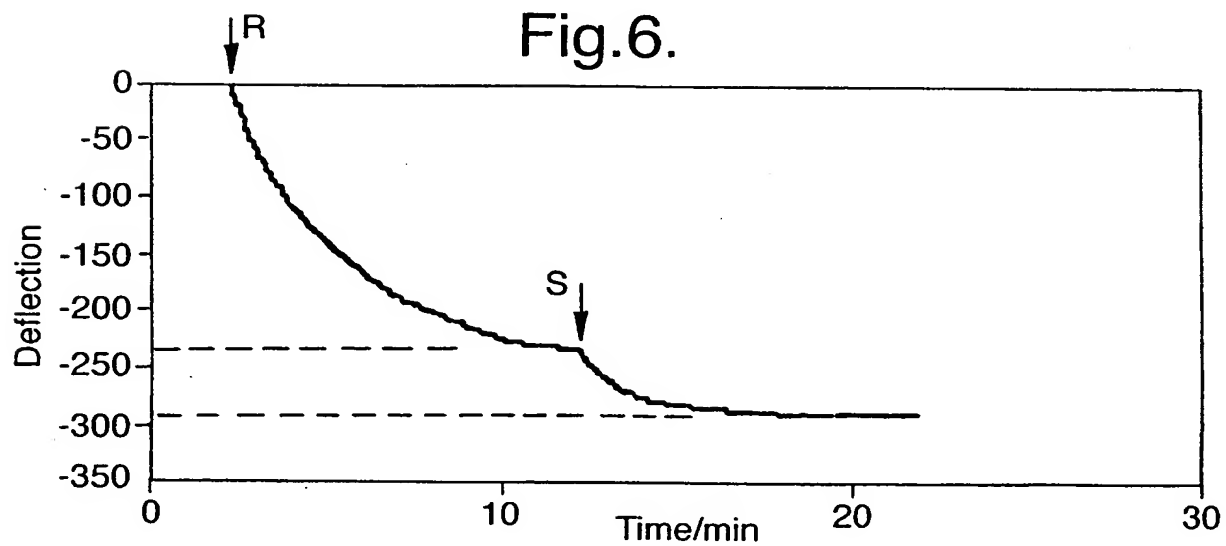

INTERNATIONAL SEARCH REPORT

International Application No
PCT/GB 99/02952

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 G01N33/543 G01N27/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 7 G01N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No
P.X	WO 98 50773 A (UNIVERSITY OF MINNESOTA) 12 November 1998 (1998-11-12) the whole document	1.4.6-10
X	US 5 719 324 A (T. G. THUNDAT ET AL.) 17 February 1998 (1998-02-17) column 7, line 65 - column 8, line 28 column 9, line 3 - line 9: claims	1.4-6, 8-10
X	US 5 445 008 A (E. A. WACHTER ET AL.) 29 August 1995 (1995-08-29) the whole document	1.4-10
A	EP 0 657 737 A (HEWLETT-PACKARD COMPANY) 14 June 1995 (1995-06-14) abstract page 5, line 4 - line 26 claims 1-4	1-10
-/-		

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

Special categories of cited documents

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
- "S" document member of the same patent family

Date of the actual completion of the international search

10 December 1999

Date of mailing of the international search report

21/01/2000

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl
Fax: (+31-70) 340-3016

Authorized officer

Griffith, G

Form PCT/ISA 210 (second sheet) (July 1992)

BEST AVAILABLE COPY

INTERNATIONAL SEARCH REPORT

International Application No

PCT/GB 99/02952

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category	Citation of document with indication where appropriate of the relevant passages	Relevant to claim No
A	<p>E.-L. FLORIN ET AL.: "Adhesion forces between individual ligand-receptor pairs." SCIENCE..</p> <p>vol. 264, 15 April 1994 (1994-04-15), pages 415-417, XP002125201</p> <p>AMERICAN ASSOCIATION FOR THE ADVANCEMENT OF SCIENCE. WASHINGTON, DC..</p> <p>US</p> <p>ISSN: 0036-8075</p> <p>cited in the application</p> <p>the whole document</p> <p>-----</p>	1-10

Form PCT/ISA/210 (continuation of second sheet) (July 1992)

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/GB 99/02952

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 9850773	A	12-11-1998	NONE	
US 5719324	A	17-02-1998	NONE	
US 5445008	A	29-08-1995	NONE	
EP 657737	A	14-06-1995	US 5527711 A JP 7209166 A	18-06-1996 11-08-1995